

# ALDOB N334K ToolSet™ for LightCycler™ (Aldolase B, Hereditary Fructose Intolerance)

Lyophilized ToolSet for PCR using the LightCycler™ Instrument. Licensed by Roche Diagnostics GmbH

**Order#: ALDOB 334 - 16**

1 ToolSet for 16 reactions

Store at 4°C, protected from light.  
Exposure to light may especially damage  
the Oligotool™ tube (vial with red cap).

For use with LightCycler-DNA Master Hybridization Probes, 10 x conc. (Roche Cat.No.: 2 015 102)

## 1. ToolSet contents

Vial	Label	Content	Quantity
			<b>ALDOB 334 - 16</b>
<b>1, Red cap</b>	<b>OligoTool</b>	- lyophilized oligos for PCR - contains mutation detection and anchor probe, primers	For 16 tests  Dissolved: 50 µL
<b>2, Green cap</b>	<b>Control</b>	- lyophilized wild type DNA	Dissolved: 20 µL
<b>3, Blue cap</b>	<b>Solvent</b>	- to dissolve OligoTool / Control	1000 µL of Solvent

Additional equipment and reagents required but not supplied :  
LightCycler-DNA Master Hybridization Probes, 10 x conc.Cat.No.: 2 015 102, including 25mM MgCl<sub>2</sub>; LightCycler  
instrument, LightCycler capillaries, DNA extraction materials

## 2. Introduction

### 2.1. Product overview

#### ToolSet description

This ToolSet is specifically designed for genotyping the N334K polymorphism (C3925G at nt level) in the Aldolase B (ALDOB) gene by LightCycler PCR with Melting Curve Analysis. Primer pair and fluorescent detection and anchor probes have been optimized for specific amplification of a 119 bp segment containing the potentially mutated site and optimal genotype discrimination.

#### Control material

Wild type control DNA, lyophilized.

#### Storage of ToolSet and Solutions

Store at +4°C when lyophilized, protected from light.  
The unopened lyophilized ToolSet is stable at +4°C for 12 months from date of  
manufacture if protected from light. When dissolved store at +4°C for a maximum  
of 4 weeks, or at -20°C for longer periods (months), protected from light.  
Avoid freezing and thawing.

### 3. Preparation for LightCycler PCR

**Toolset preparation** **Dissolve** the content of the **OligoTool** tube (Red Cap) with **50 µl of Solvent**.  
**Dissolve** the content of the **Control** tube (Green Cap) with **20 µl of Solvent**.

1. Before opening tubes, centrifuge them quickly.
2. Add Solvent into OligoTool tube and Control tube as above.
3. Recap tubes, vortex gently.
4. Before opening tubes, centrifuge them quickly.
5. Proceed to Reaction Mix preparation.

**Primers ?** You don't have to add primers.  
**Probes ?** You don't have to add probes.

**Reaction Mix Preparation** For 1 (One) reaction, prepare the Reaction Mix as shown in the following table :

Reagent	µL
OligoTool ALDOB 334 -16, dissolved	2.8
Solvent ALDOB 334 -16	<b>8.8</b>
MgCl <sub>2</sub> 25 mM	<b>2.4 (final 4 mM)</b>
Master Hybridization Probes 10x	2
Total Reaction Mix	16
+ Your DNA or Control ALDOB 334 -16	4
Grand Total	20

Use Master Hybridization Probes 10x and MgCl<sub>2</sub> 25 mM from Roche LightCycler-DNA Master Hybridization Probes, 10 x conc. (Roche Cat.No.: 2 015 102, including 25mM MgCl<sub>2</sub>).  
 For multiple reactions, multiply the indicated volumes appropriately.

**Positive Control** Always run a positive control with the samples. Use the dissolved ALDOB NN334 wild type Control DNA (Green Cap).

**Negative control** Always run a negative control with the samples. To prepare a negative control, replace the template DNA with Solvent (Blue Cap).

**Extraction of genomic DNA** You can use different Kits for DNA isolation, either with a manual method or with an automated system. The elution buffers should be salt-free. Example : Roche High Pure PCR Template Preparation Kit (Cat.No. 1 796 828).

**Application** The **ALDOB N334K** ToolSet™ for LightCycler™ allows detection of the **C→G** mutation at position 3925 in the ALDOB gene resulting in the **Asn 334 Lys** exchange in the Aldolase B protein causing a **loss of enzymatic activity**. **The homozygous 334 Lys mutant of Aldolase B is a frequent cause of Hereditary Fructose Intolerance**.

Note : In parts of the scientific literature this mutation is also designated as N335K due to different amino acid numbering.

Note : This ToolSet was developed for use in life science research only.

Note : This ToolSet uses the same Time-Temperature Protocol as the ALDOB A149P and ALDOB A174D ToolSets and can therefore be used in the same run.

## 4. LightCycler Settings and Experimental Protocol

### Denaturation

Cycle Program Data	Value
Cycles	1
Analysis Mode	None
Temperature Targets	<b>Segment 1</b>
Target Temperature (°C)	95
Incubation time (s)	30
Temperature Transition Rate (°/s)	20
Secondary Target Temperature (°C)	0
Step Size (°C)	0
Step Delay (Cycles)	0
Acquisition Mode	None

### Amplification

Cycle Program Data	Value		
Cycles	<b>45</b>		
Analysis Mode	None		
Temperature Targets	<b>Segment 1</b>	<b>Segment 2</b>	<b>Segment 3</b>
Target Temperature (°C)	95	<b>55</b>	72
Incubation time (s)	1	<b>10</b>	8
Temperature Transition Rate (°/s)	20	20	<b>3</b>
Secondary Target Temperature (°C)	0	0	0
Step Size (°C)	0	0	0
Step Delay (Cycles)	0	0	0
Acquisition Mode	None	Single	None

### Melting Curve Analysis

Cycle Program Data	Value		
Cycles	1		
Analysis Mode	Melting Curves		
Temperature Targets	<b>Segment 1</b>	<b>Segment 2</b>	<b>Segment 3</b>
Target Temperature (°C)	95	<b>36</b>	<b>85</b>
Incubation time (s)	60	60	0
Temperature Transition Rate (°/s)	20	20	0.2
Secondary Target Temperature (°C)	0	0	0
Step Size (°C)	0	0	0
Step Delay (Cycles)	0	0	0
Acquisition Mode	None	None	Continuous

### Cooling

Cycle Program Data	Value
Cycles	1
Analysis Mode	None
Temperature Targets	<b>Segment 1</b>
Target Temperature (°C)	40
Incubation time (s)	30
Temperature Transition Rate (°/s)	20
Secondary Target Temperature (°C)	0
Step Size (°C)	0
Step Delay (Cycles)	0
Acquisition Mode	None


### LC Program Version and Fluorescence Display Mode

Developed with LC Program Version 3.5 and automatic gain control.  
For fluorescence display use F2/F1, or F2 with colour compensation.

## 5. Typical results

### Introduction

Use the Melting Curve program to genotype the human genomic DNA research samples. The melting peaks allow discrimination between the possible genotypes at the **N334K** mutation site in the **ALDOB** gene. Figure 1 shows a typical result obtained with the **ALDOB N334K ToolSet™** for LightCycler™ :

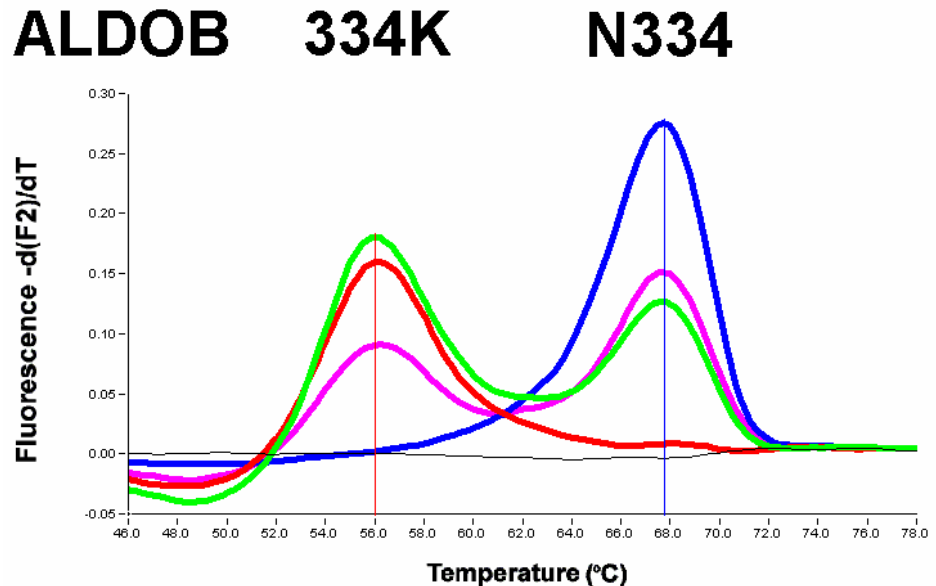

**Figure 1 : Melting curve analysis of genotypes at AA position 334 of the human ALDOB gene**

**BLUE :** Homozygote NN334 wild type DNA (Control DNA contained in the ToolSet)  
**GREEN :** Heterozygote N334K plasmid DNA  
**RED :** Homozygote mutant 334KK DNA  
**PINK :** 1:1 Mix of Homozygote NN334 wild type DNA and Homozygote mutant 334KK DNA  
**BLACK :** No DNA Control.

**Blue Cursor :**  $T_m = 67.7\text{ }^\circ\text{C}$  ; **Red Cursor :**  $T_m = 56.0\text{ }^\circ\text{C}$

Conditions : LC program version 3.5 with automatic gain setting, Color compensation and Digital Filter enabled, Degrees to average : 8.0. Calculation Method : Polynomial.

**Note :** The values for the respective melting temperatures may vary for +/- 2.5 °C between different experiments. The Delta T between the melting peaks for different genotypes may vary +/- 1.0 °C. The ALDOB N334K ToolSet™ has been developed for and validated with the LightCycler™ and its original accessory materials and reagents. Performance of the ToolSet with other instruments, accessories and reagents has not been validated by ratiogen.

### 7. Notices to Purchaser : Licenses and Trademarks, Prohibition of Resale

ratiogen's ToolSets™ for LightCycler™ are produced and marketed under license from Roche Diagnostics GmbH. The purchase of this product does not convey any right for its use in clinical diagnostics. No license to use the PCR process is conveyed expressly or by implication by purchase of this product. The LightCycler technology is licensed from Idaho Technology Inc., Idaho Falls, ID, USA. LightCycler and High Pure are trademarks of members of the Roche group. Resale of ratiogen's products is expressly prohibited.

### How to contact ratiogen

E-mail [info@ratiogen.com](mailto:info@ratiogen.com)

Internet <http://www.ratiogen.com>